


TSH A1:D100

Filter: No filter

Last updated 10 november 2022 at 16:02 by Sjoerd van den Berg

Descriptives

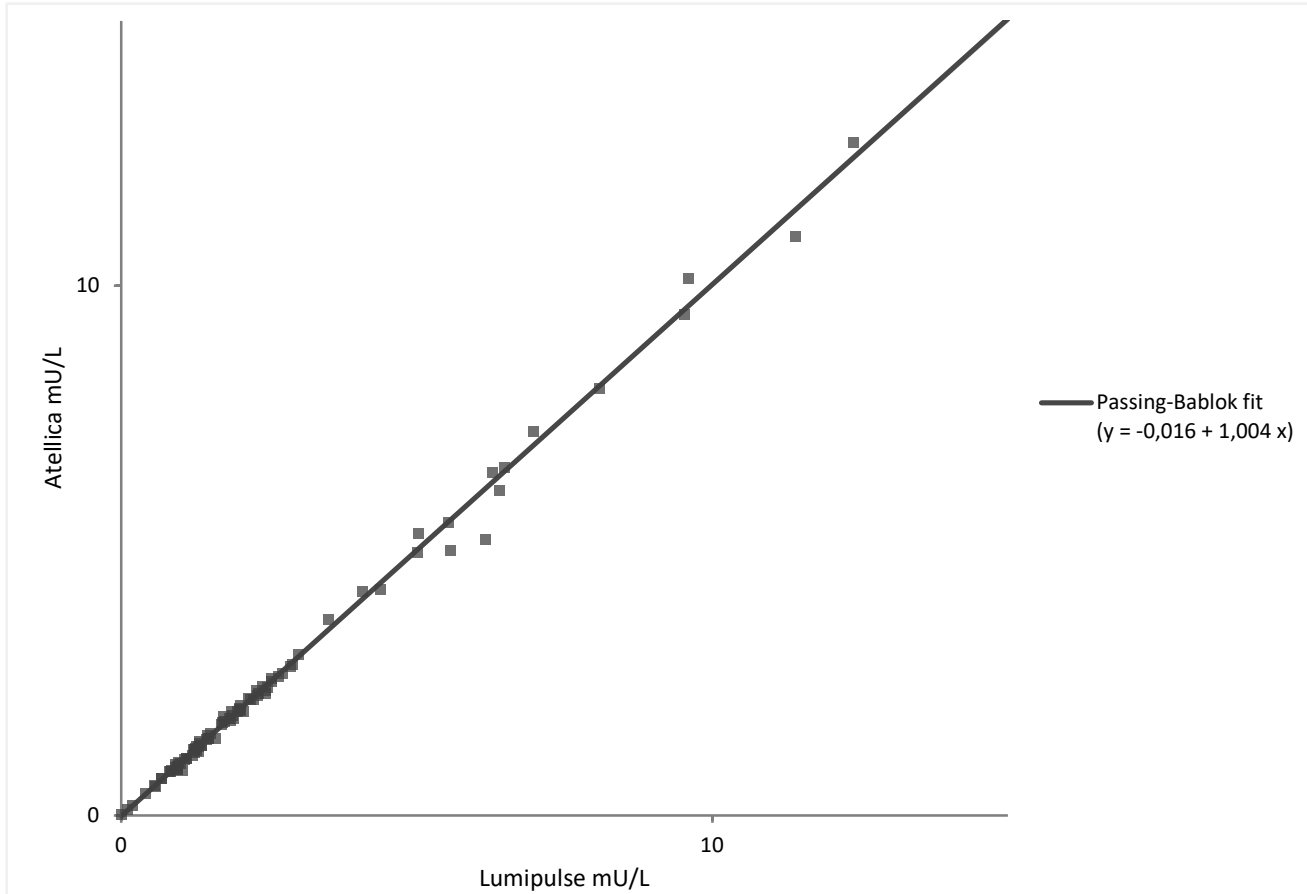

N | 91

	Minimum	Maximum
Lumipulse mU/L	0,0070	56,0000
Atellica mU/L	0,0090	62,7820

Fit Y on X

Passing-Bablok fit

Equation | Atellica mU/L = -0,016 + 1,004 Lumipulse mU/L

Parameter	Estimate	Bootstrap 95% CI
Intercept	-0,01600	-0,04263 to 0,001167
Slope	1,004	0,9891 to 1,025

CI based on 999 bootstrap samples.